





## QUICK PAIRING GUIDE

# Pairing the iChoice Pulse Oximeter with MyLife365 Smart Devices

 Follow Manufacturer Instructions for Use.  
*Still have questions or need assistance? Contact  
Support at [support@life365.health](mailto:support@life365.health)*


# Pairing the iChoice Pulse Oximeter with MyLife365 Smart Devices

1 After assigning a smart device to a member, select the Reminders application. You will receive two prompts, select “**ALLOW**” for both prompts.




**This step must be completed before pairing Bluetooth Devices.**

2 Select the Bluetooth Icon\*.  
Enter the password “**3651**” and select “**OK**”.





*\*the Bluetooth App Icon location may vary by device*

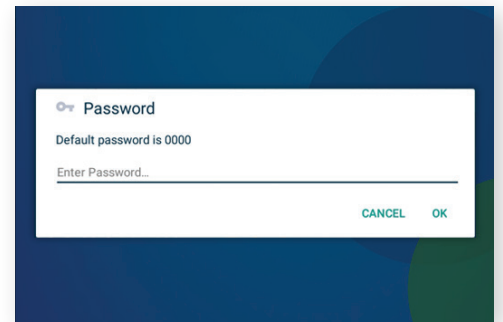

3 On the “**My Devices**” page, select “**Add New**” (A).

The smart device will search for the Bluetooth device.

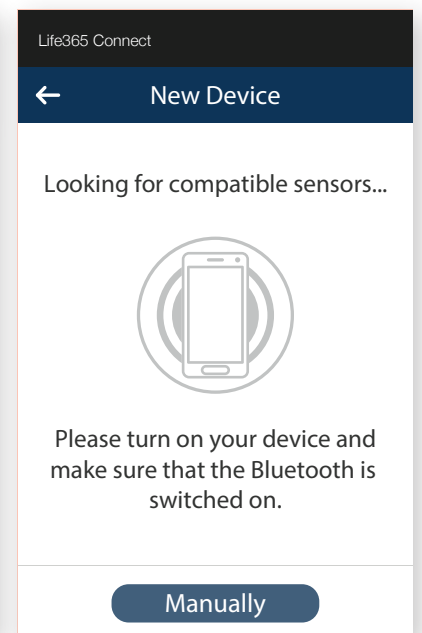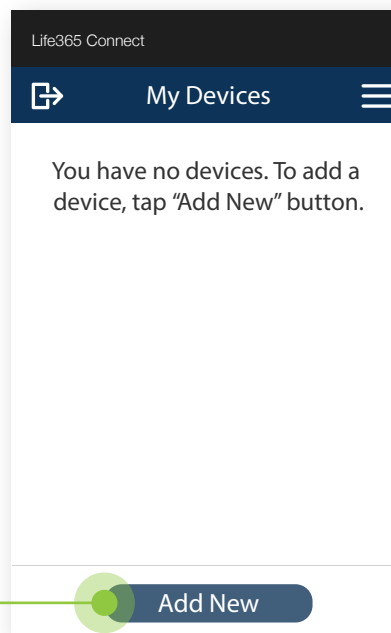

# Pairing the iChoice Pulse Oximeter with MyLife365 Smart Devices

4



To pair, take a test reading

Turn on the pulse oximeter by pressing the power button.

Insert index finger tip into the device. After reading displays on the meter, remove finger.

5


Once found, select the Bluetooth device name (B).

Select "Add to My Devices" (C).

*This is an example. Device name displayed will reflect the Bluetooth device the user is attempting to pair.*

6

Device pairing is now complete.

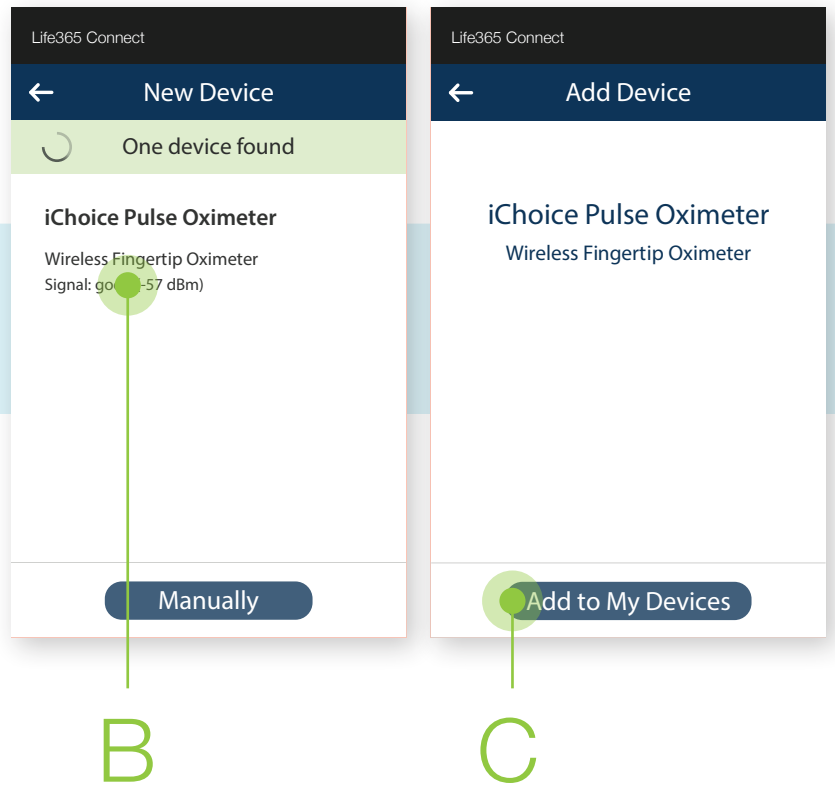



# MANUAL PAIRING:

## Difficulty pairing this device?

- 1 Try manually pairing the device by selecting “**Add New**” on the “**My Devices**” page (A), then selecting “**Manually**” (B).
- 2 Search for the device by Manufacturer by selecting the magnifying glass (C).
- 3 Select the device, then select “**Add to My Devices**”.

Device pairing is now complete.

Take a test reading with the device.  
Hub will announce the reading.

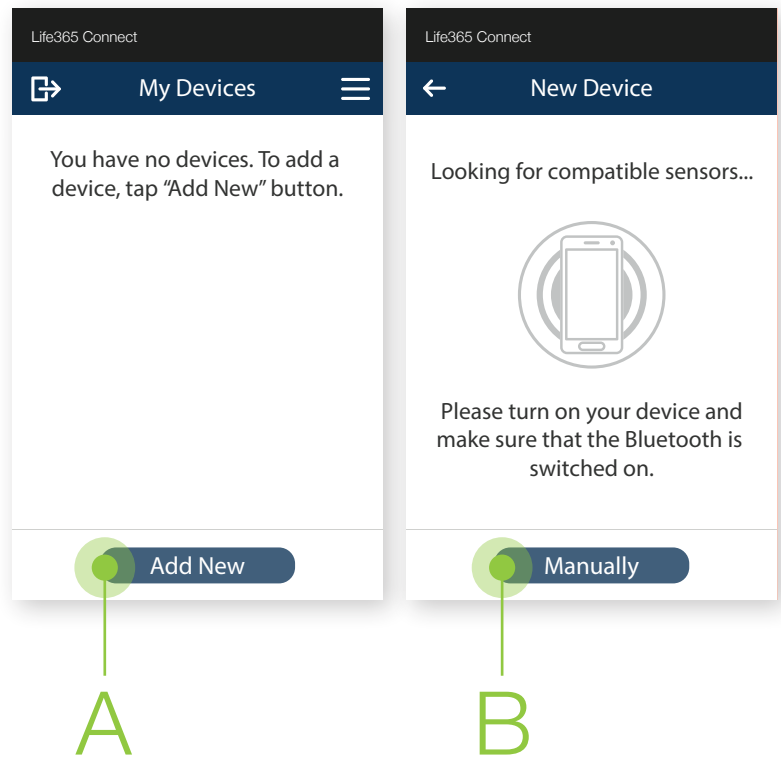


### NOTE:

The Reminders Application must be opened BEFORE opening the Bluetooth Application. If the Bluetooth Application is opened before the Reminders Application, a “**Choose Server Location**” error screen will display.

If this error screen is shown:

1. Exit the Bluetooth Application
2. Enter the Reminders Application
3. Accept both prompts
4. Re-enter the Bluetooth Application
5. Select the Refresh symbol (D).



**You can now complete device pairing.**